

Protocol for density gradient centrifugation of Porcine sperm


Materials required

- **PorciPure™** Top & Bottom Layer • Dispensing pipette and disposable tips
- **PorciWash™** • Pasteur pipettes
- Conical centrifuge tubes • Centrifuge with swing-out rotor

Protocol

Depending on the volume ejaculate to process, different sizes of tubes can be used. See table below.

Ejaculate size	Tube size (mL)	Bottom layer Volume (mL)	Top layer Volume (mL)	Ejaculate volume (mL) on the gradient
Small	10-15	2	2	1,5
Medium	50	5	5	3-4
Large	50	10	10	7-8

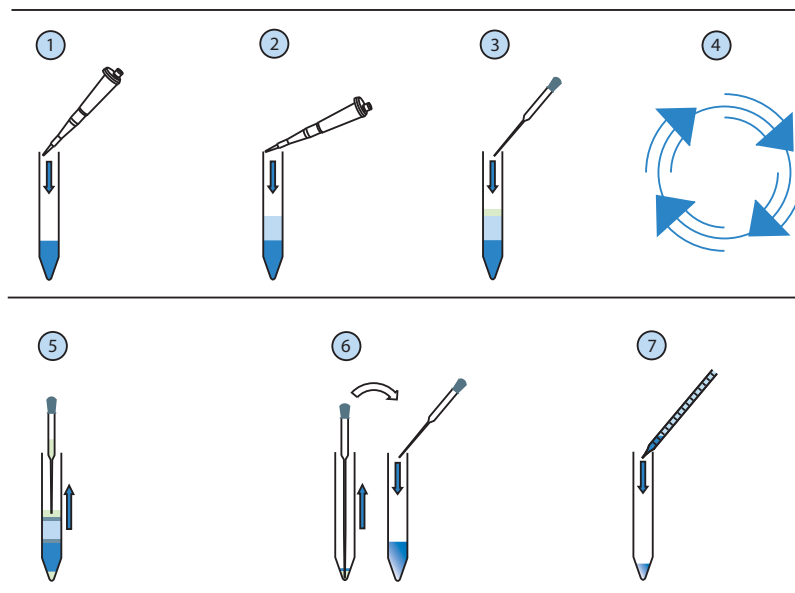

- Bring all materials to room temperature.
- Extend the ejaculate with **PorciWash™** (max conc 250 million/mL).

1. Using a sterile pipette, transfer **PorciPure™** Bottom Layer to a conical centrifuge tube (see volumes and sizes above).
2. Using a new sterile pipette, layer **PorciPure™** Top Layer carefully over the **PorciPure™** Bottom Layer, taking care not to disrupt the gradient layers.
3. Layer extended semen on top of the gradient taking care not to disrupt the layers.
4. Centrifuge at 300 g for 20 minutes at room temperature in a centrifuge with a swing-out rotor.
5. Carefully remove ejaculate, **PorciPure™** Top Layer and most of the **PorciPure™** Bottom Layer.
6. Using a **new** sterile pipette, transfer and resuspend sperm pellet in 1 mL **PorciWash™** in a new sterile tube (10-15 mL).
7. Dilute to desired concentration with **PorciWash™**.

Note: we recommend preparing two **PorciPure™** gradients for each sample, to reduce the risk of overloading a single gradient and to provide two tubes to balance the centrifuge rotor.